



BD_FACSAriaII-1_13-COLOR_85um_nozzle

Cytometer:	FACSAriaII	User:	Administrator
Cytometer Name:	FACSAriaII	Institution:	N/A
Serial Number:	P2230064	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	11/30/2018 3:28:43 PM
Sheath Pressure:	45.00		
Nozzle Size:	85		
Window Extension:	2.00		


Blue Laser
(488nm)
FSC

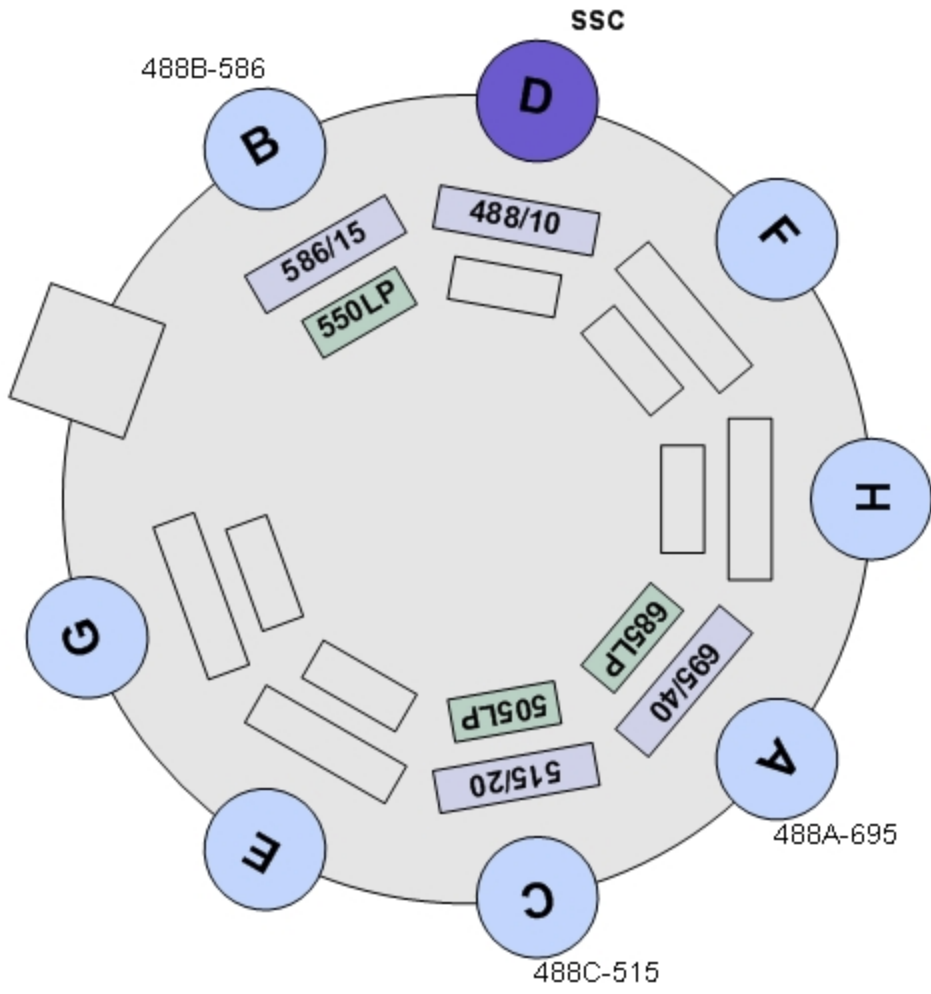


Red Laser
(633nm)

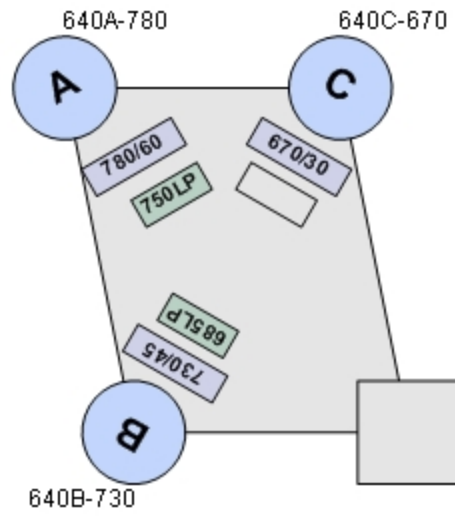

Violet Laser
(407nm)

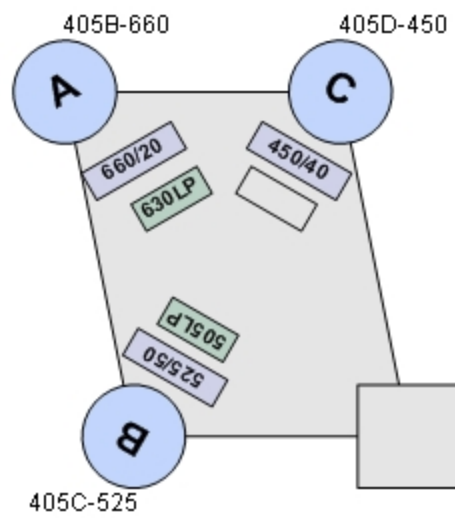

YellowGreen Laser
(561nm)

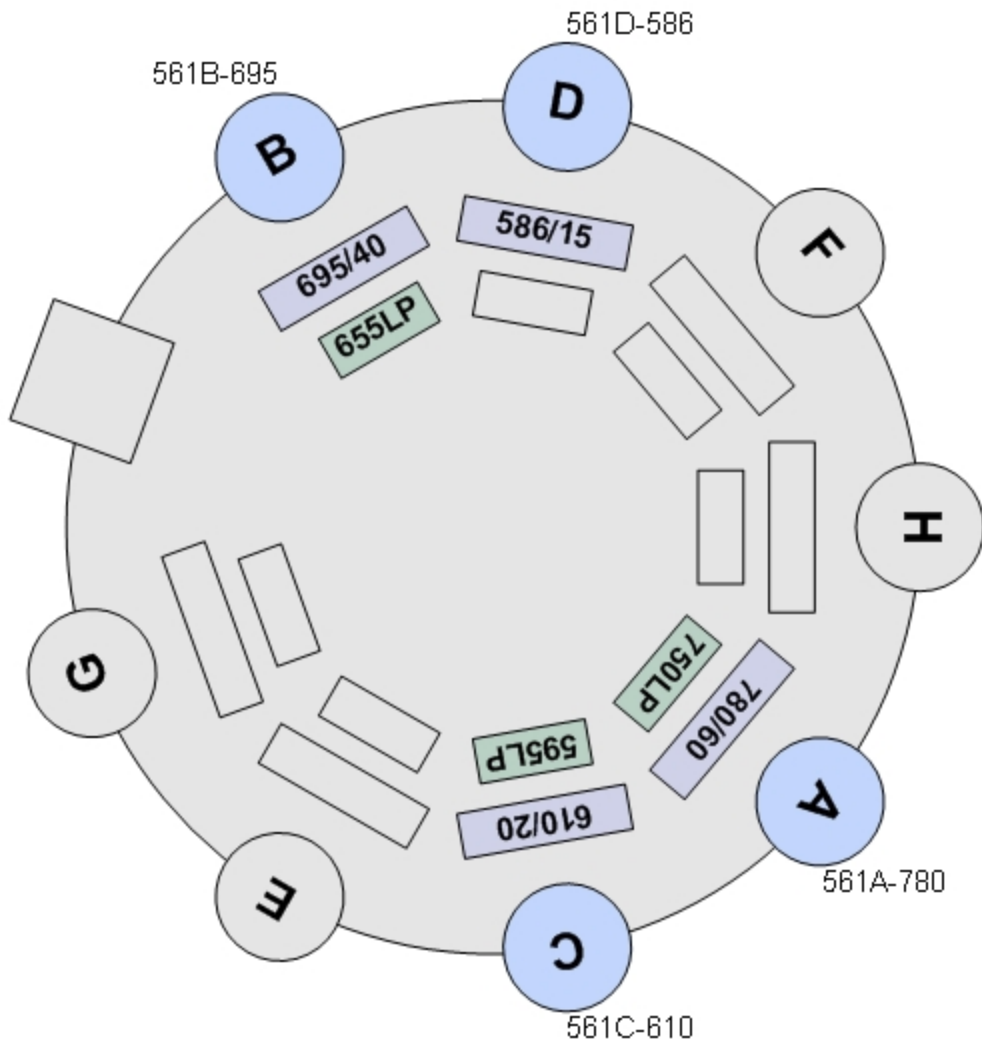

Comments: