



FACSriaII-2_16-COLOR_85um nozzle without FSC PMT

Cytometer:	FACSriaII	User:	Administrator
Cytometer Name:	FACSriaII	Institution:	N/A
Serial Number:	P69500038	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	12/21/2018 2:27:30 PM
Sheath Pressure:	45.00		
Nozzle Size:	85		
Window Extension:	2.00		


Blue Laser
(488nm)
FSC

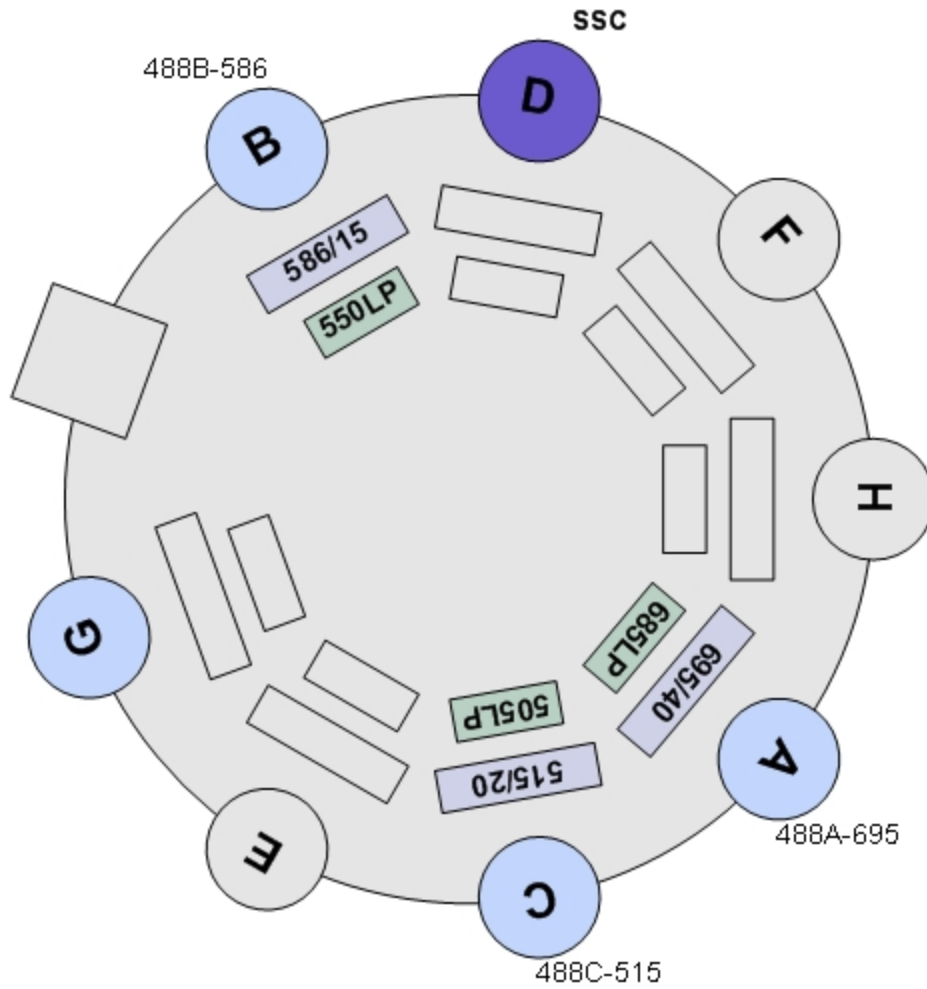


Red Laser
(640nm)

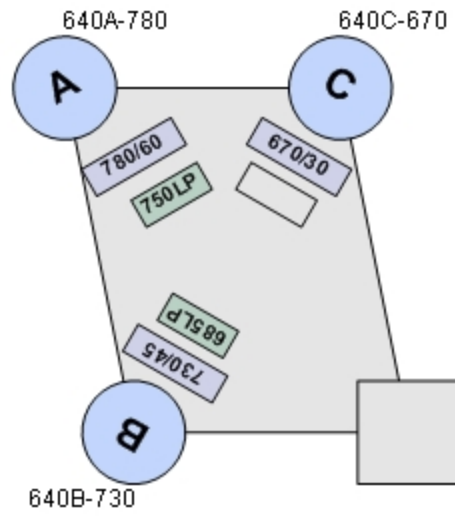


355 UV Laser
(355nm)

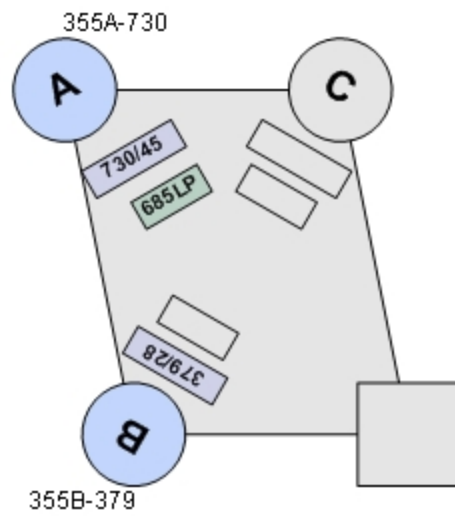

Violet Laser
(405nm)

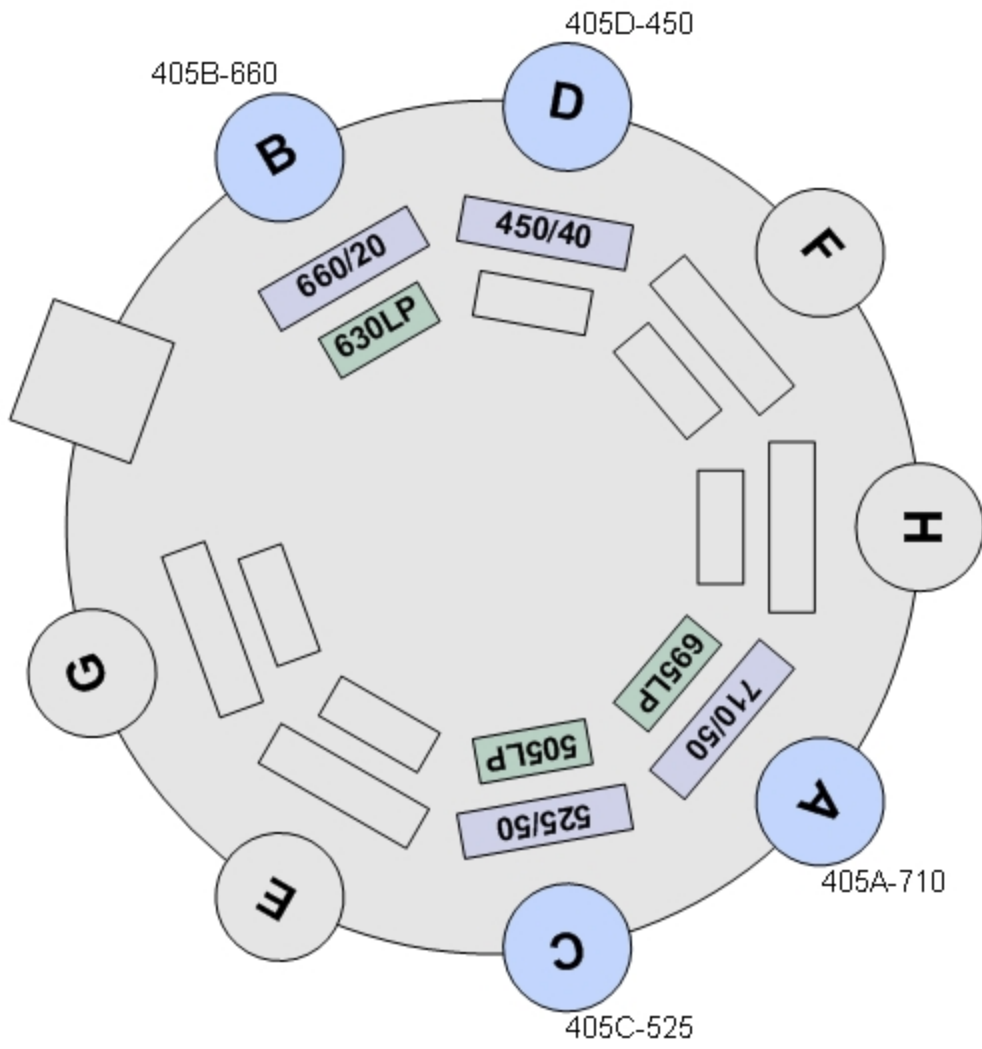

561 Yellow-Green Laser
(561nm)

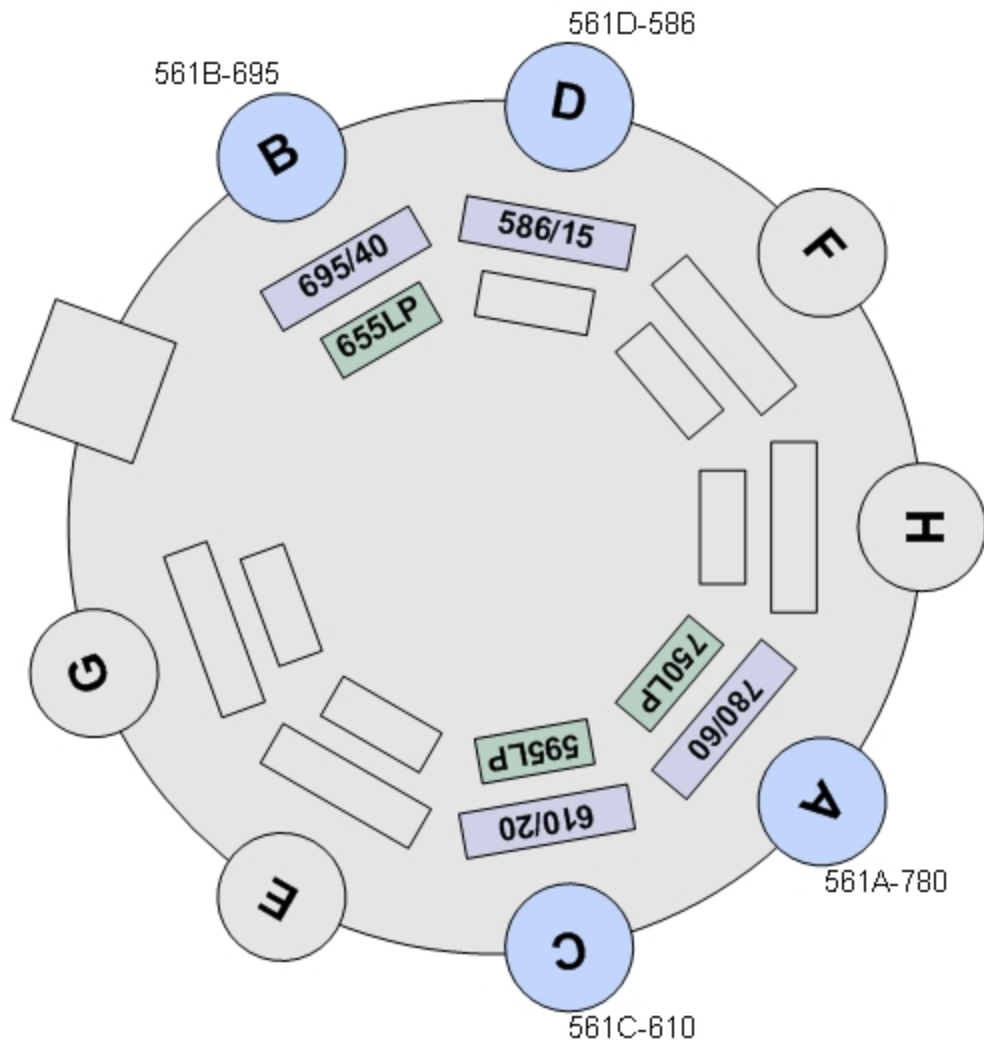

Comments: