



# BD\_FACSriaII-3\_18-COLOR\_85um\_nozzle

Cytometer:	FACSriaII	User:	Administrator
Cytometer Name:	FACSriaII	Institution:	N/A
Serial Number:	P11000011	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	11/20/2018 2:00:56 PM
Sheath Pressure:	45.00		
Nozzle Size:	85		
Window Extension:	2.00		


Blue Laser  
(488nm)  
FSC

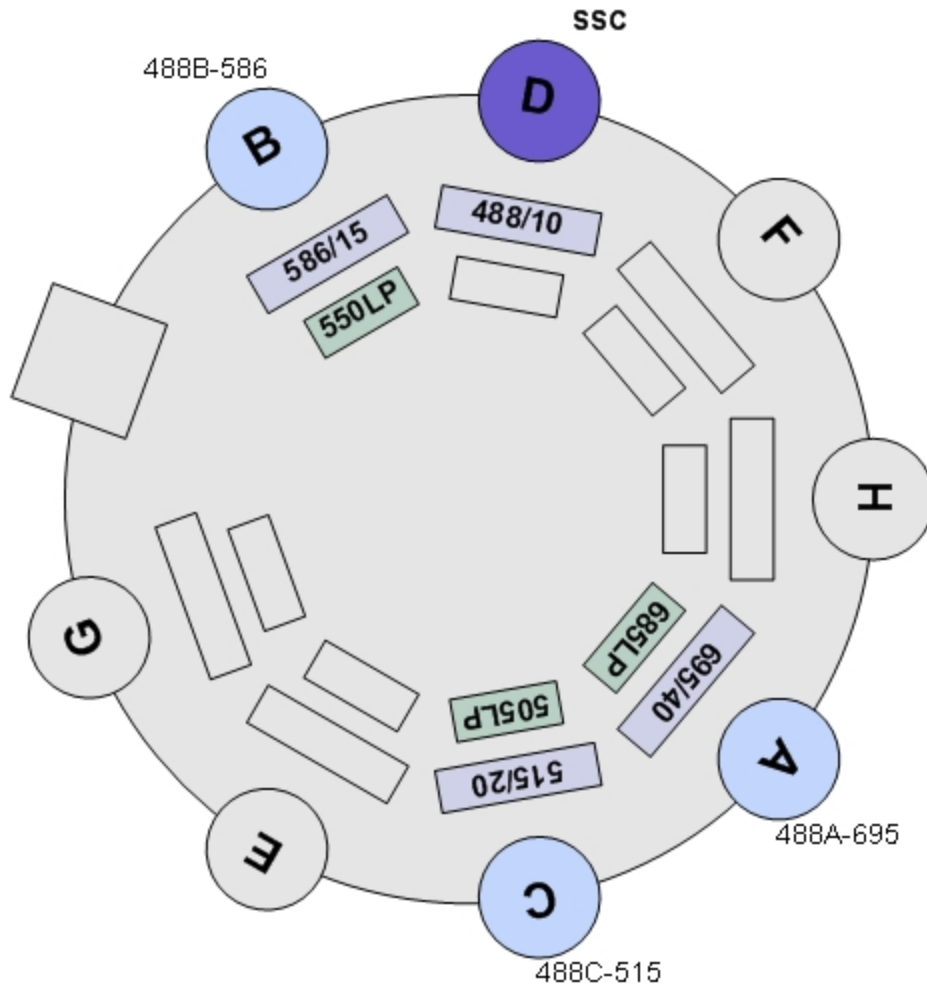


Red Laser  
(640nm)

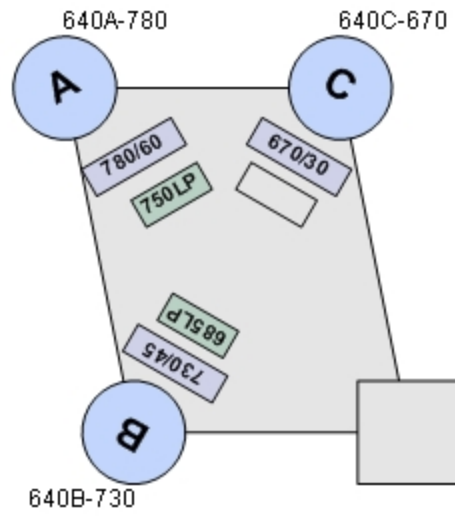


355 UV Laser  
(355nm)

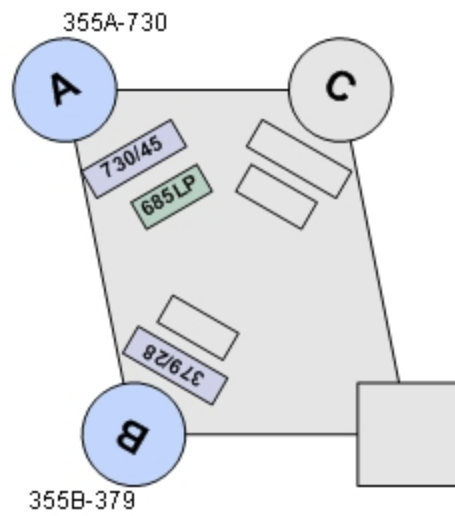


Violet Laser  
(405nm)

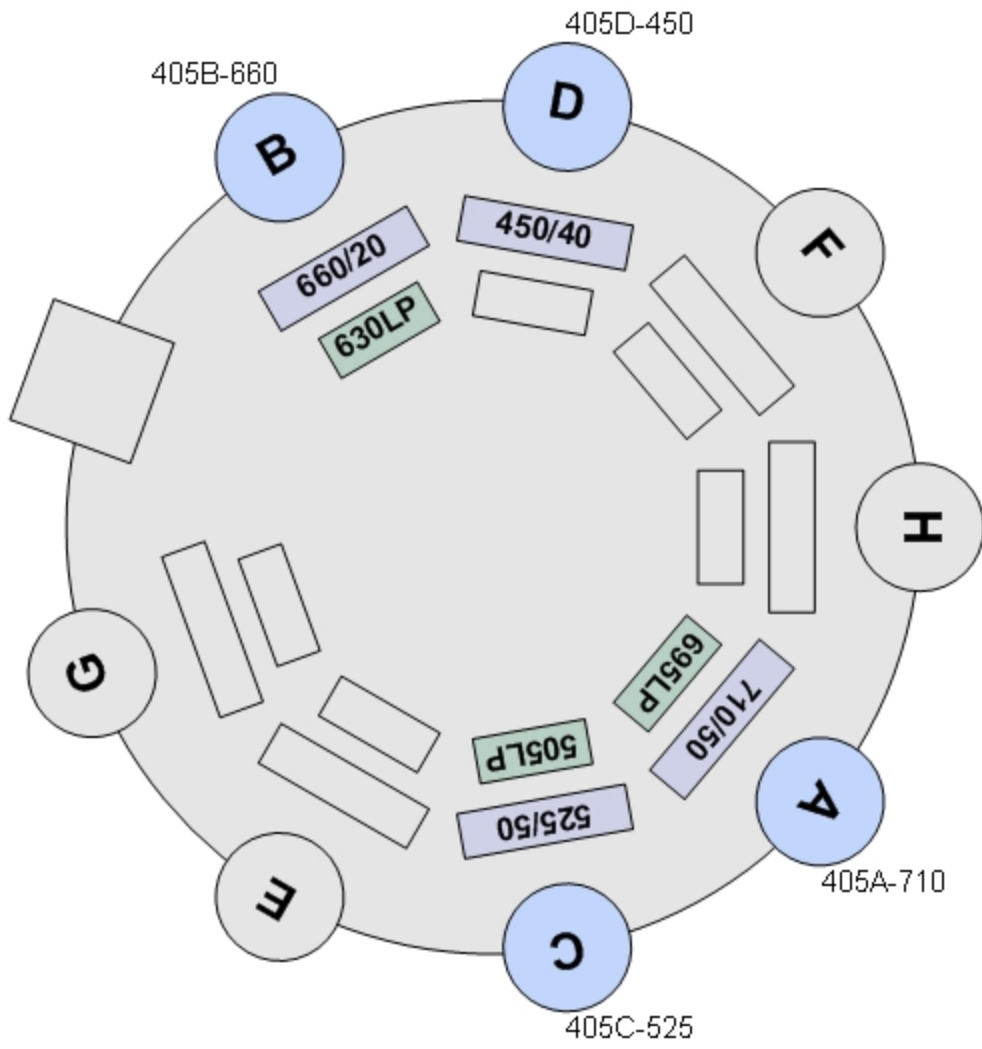

561 YellowGreen Laser  
(561nm)

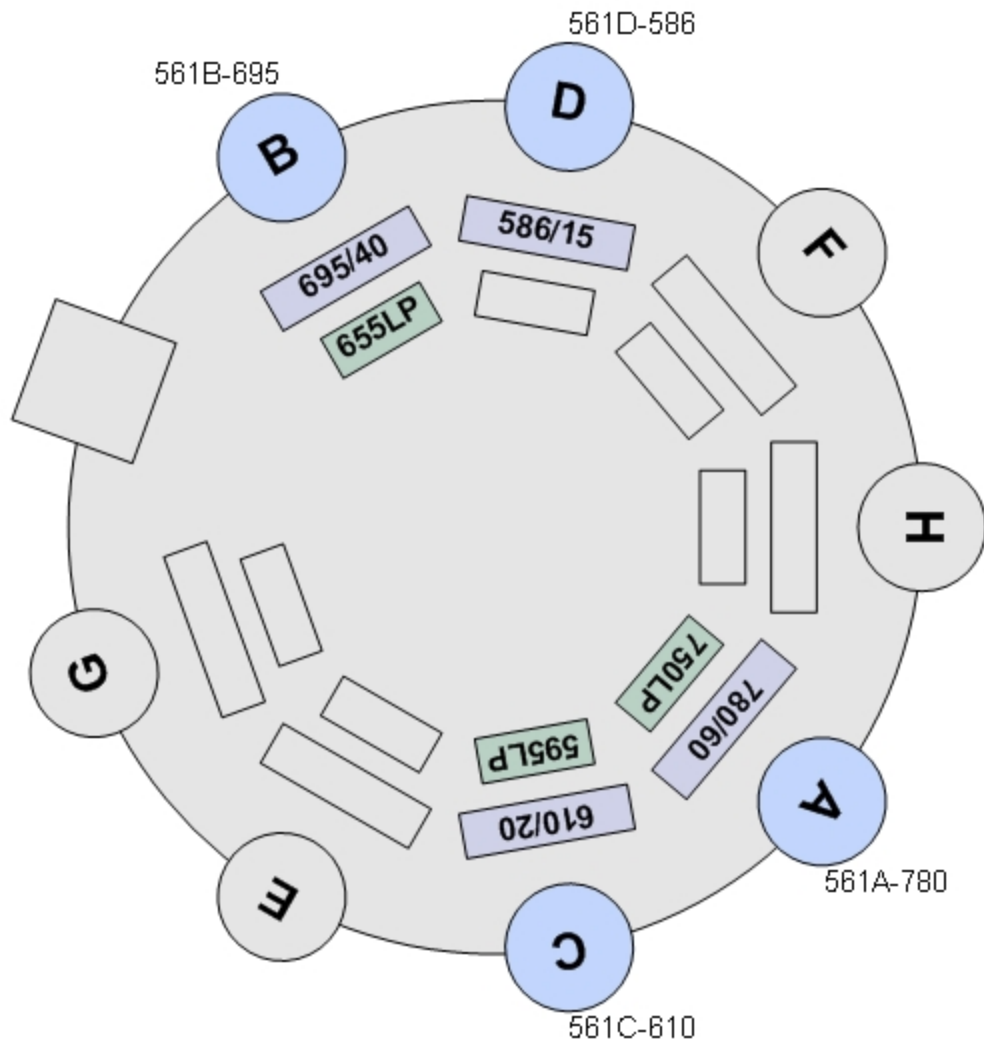

Blue Violet Laser  
(445nm)

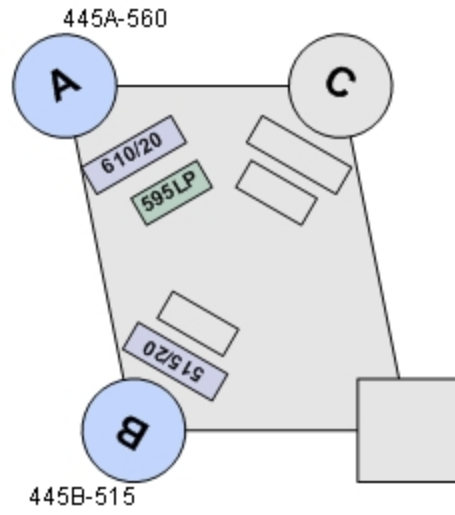

Comments: \_\_\_\_\_