



BD_LSR-Fortessa_18-COLOR_20181211

Cytometer:	LSRFortessa	User:	Administrator
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	H64780000027	Software:	BD FACSDiva 8.0.1
Input Device:	HTS	Date:	12/11/2018 2:59:48 PM
Window Extension:	10.00		


Blue Laser
(488nm)
FSC

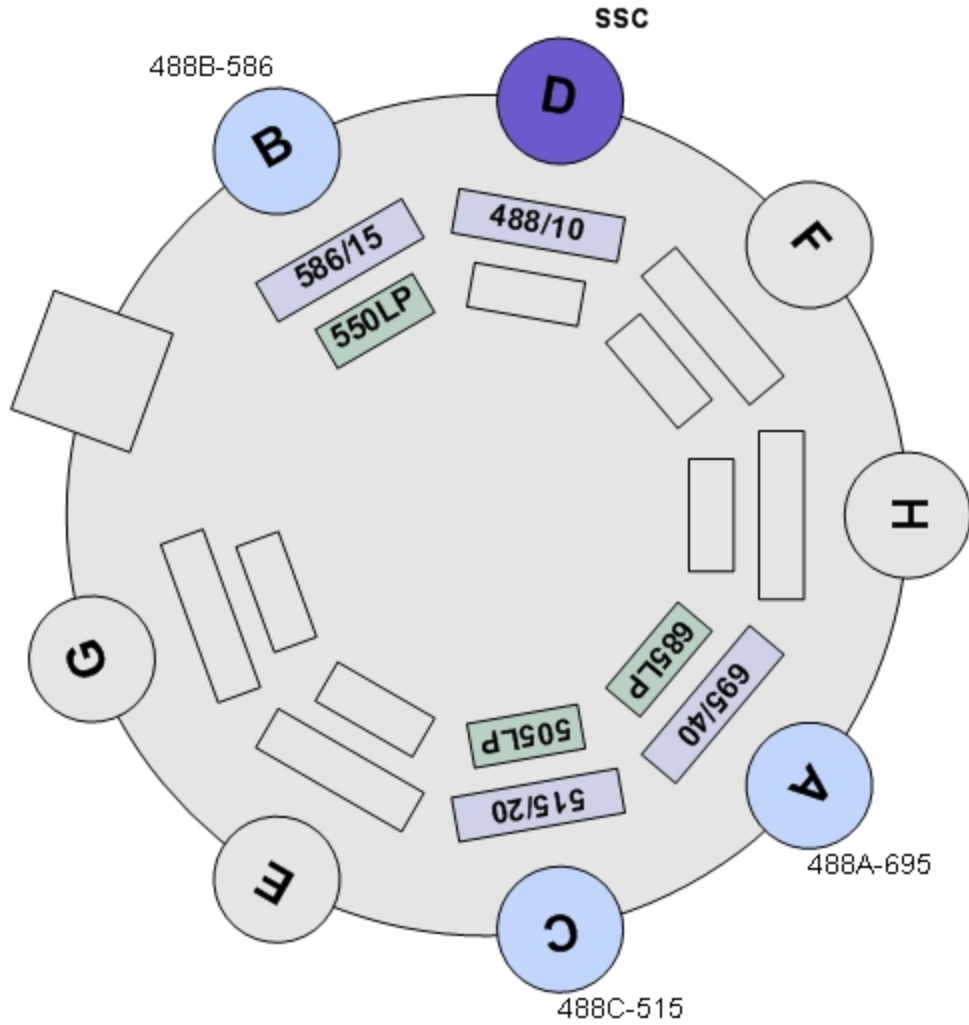


Red Laser
(640nm)

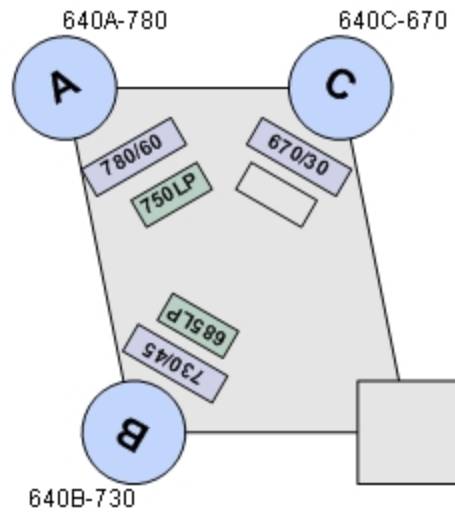


Violet Laser
(405nm)

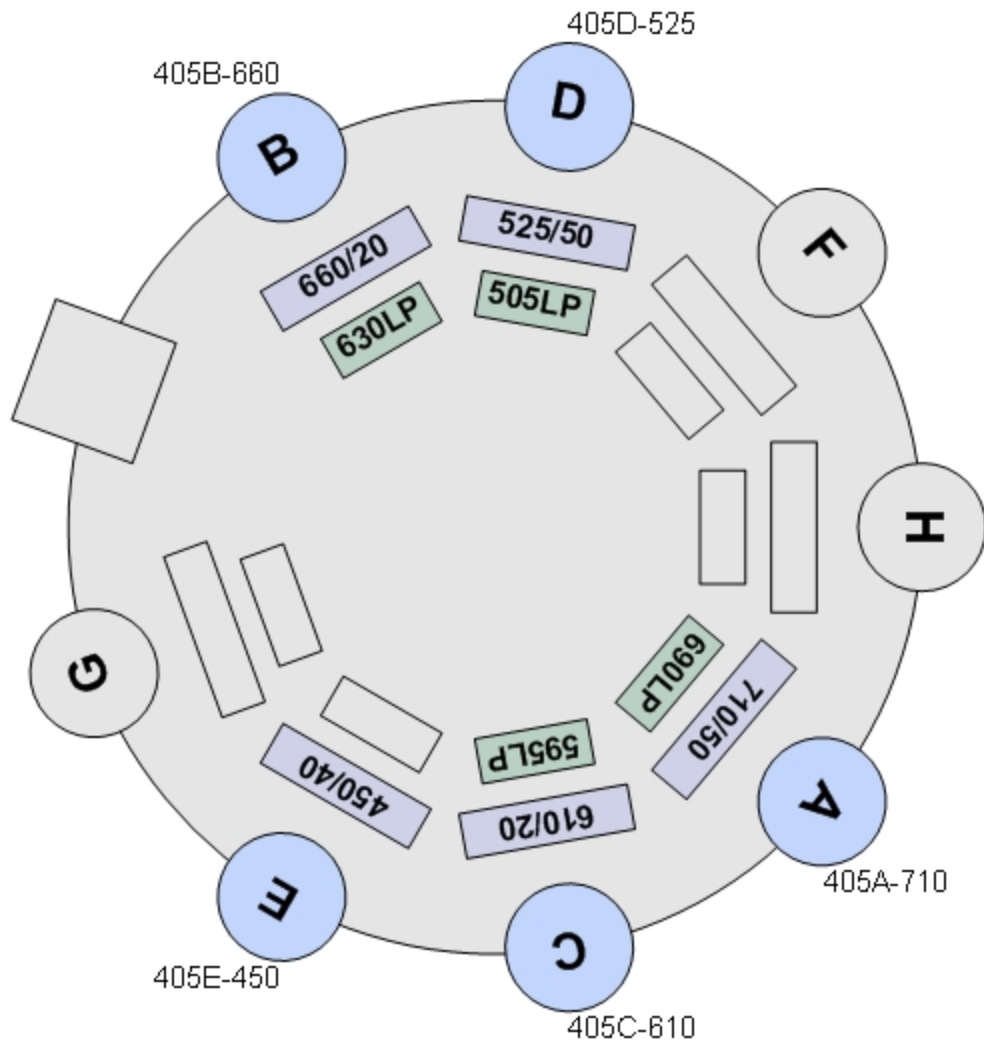

UV Laser
(355nm)

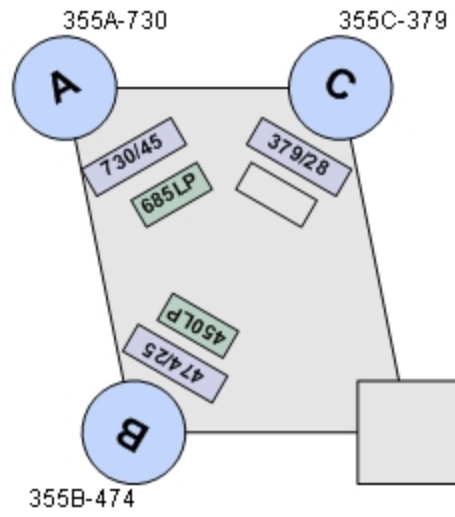

YelGr Laser
(561nm)

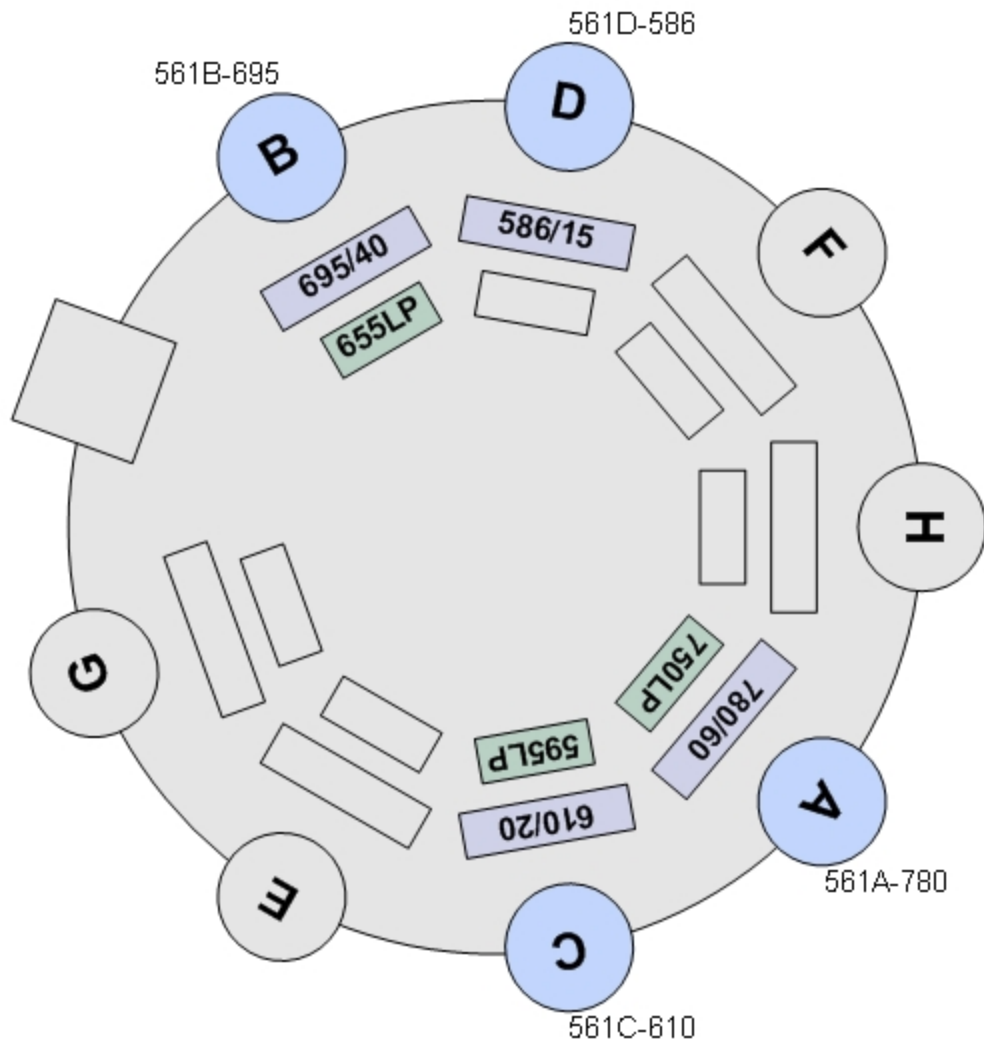

Comments: