



# BD\_LSR11-1\_16-COLOR\_20190111

Cytometer:	LSR11	User:	Administrator
Cytometer Name:	LSR11	Institution:	N/A
Serial Number:	H48200001	Software:	BD FACSDiva 8.0.1
Input Device:	HTS	Date:	1/12/2019 1:43:00 PM
Window Extension:	10.00		


Blue Laser  
(488nm)  
FSC

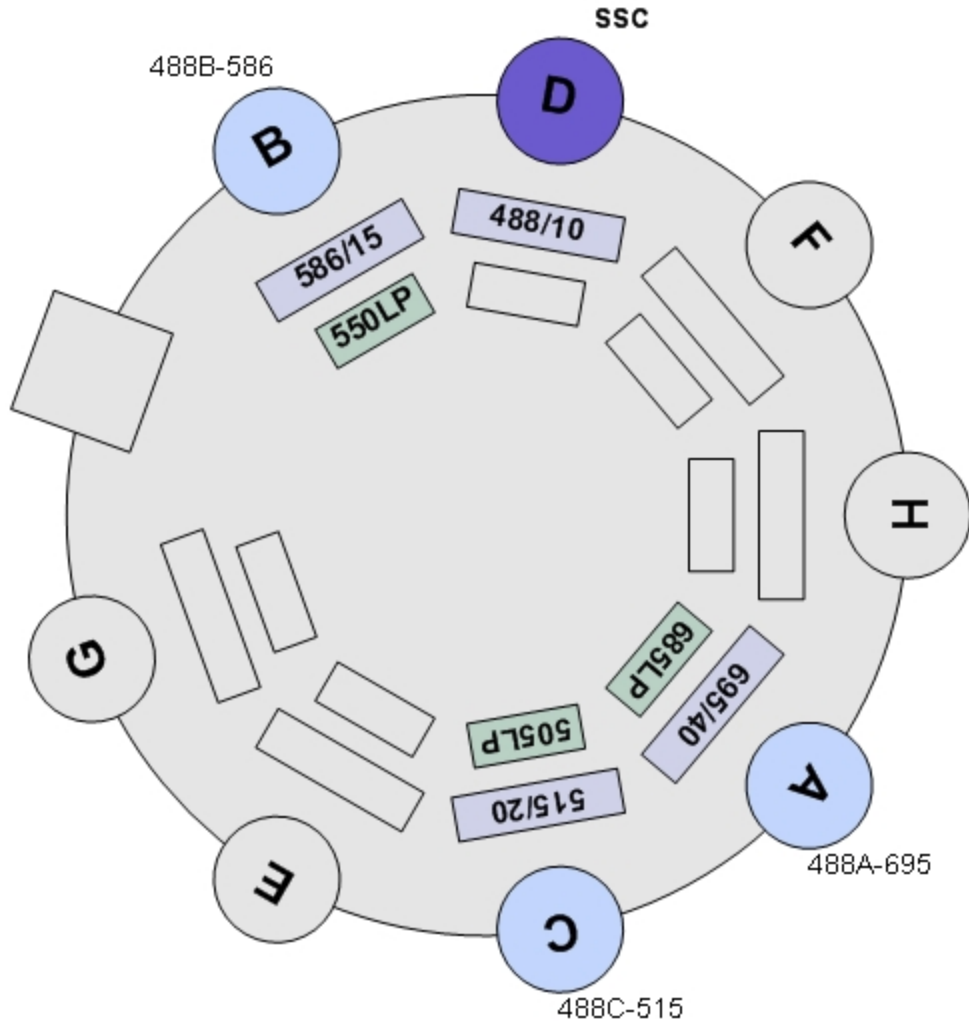


Violet Laser  
(405nm)

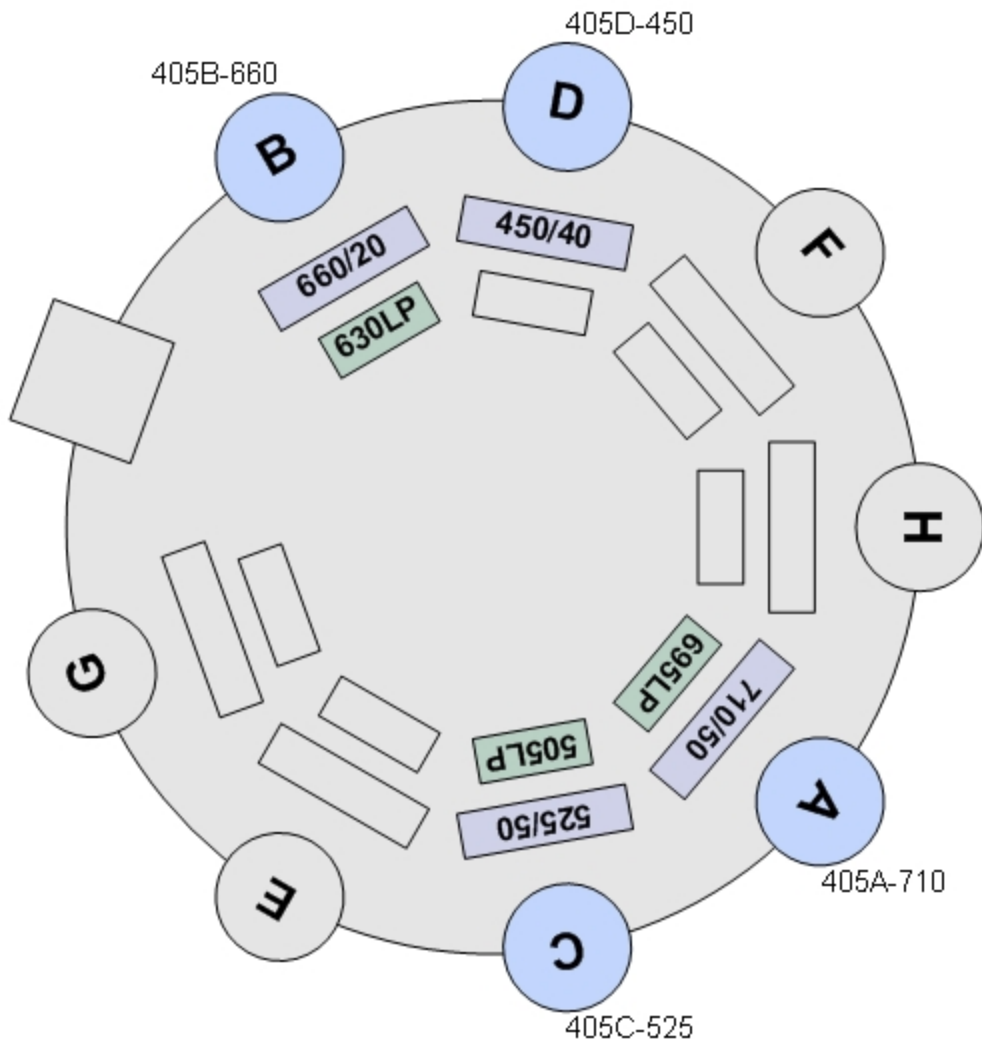


355 UV Laser  
(355nm)

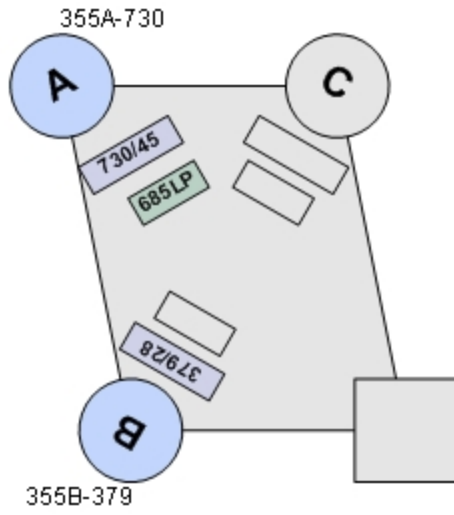

Red Laser  
(633nm)

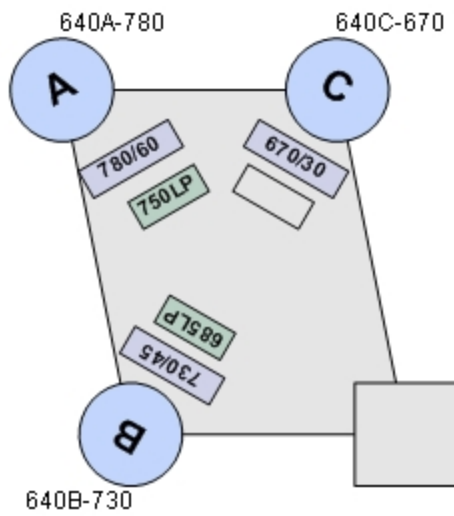

561 Yellow-Green Laser  
(561nm)

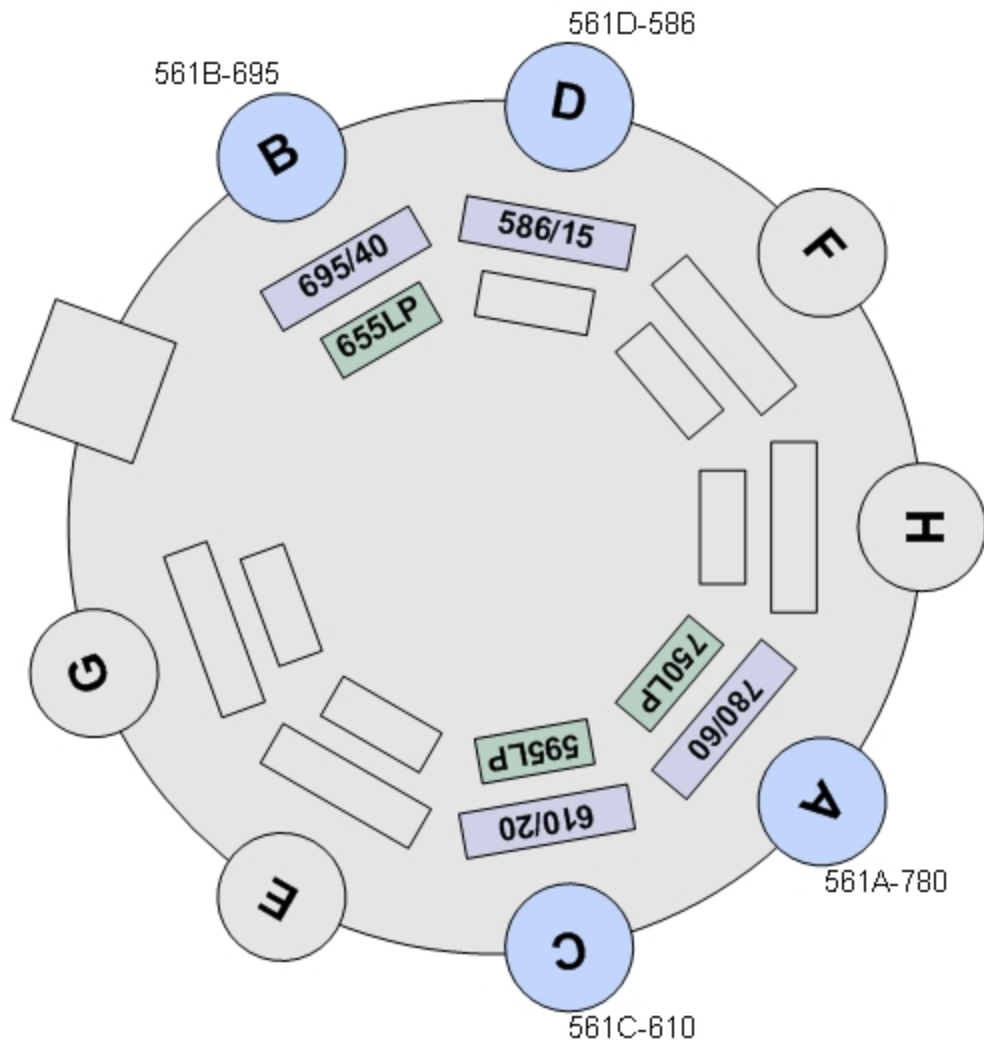

Comments: