



BD_LSR II-2_16-COLOR_20190112

Cytometer:	LSRII	User:	Administrator
Cytometer Name:	LSRII	Institution:	N/A
Serial Number:	H47100076	Software:	BD FACSDiva 8.0.1
Input Device:	HTS	Date:	1/12/2019 1:58:33 PM
Window Extension:	10.00		


Blue Laser
(488nm)
FSC

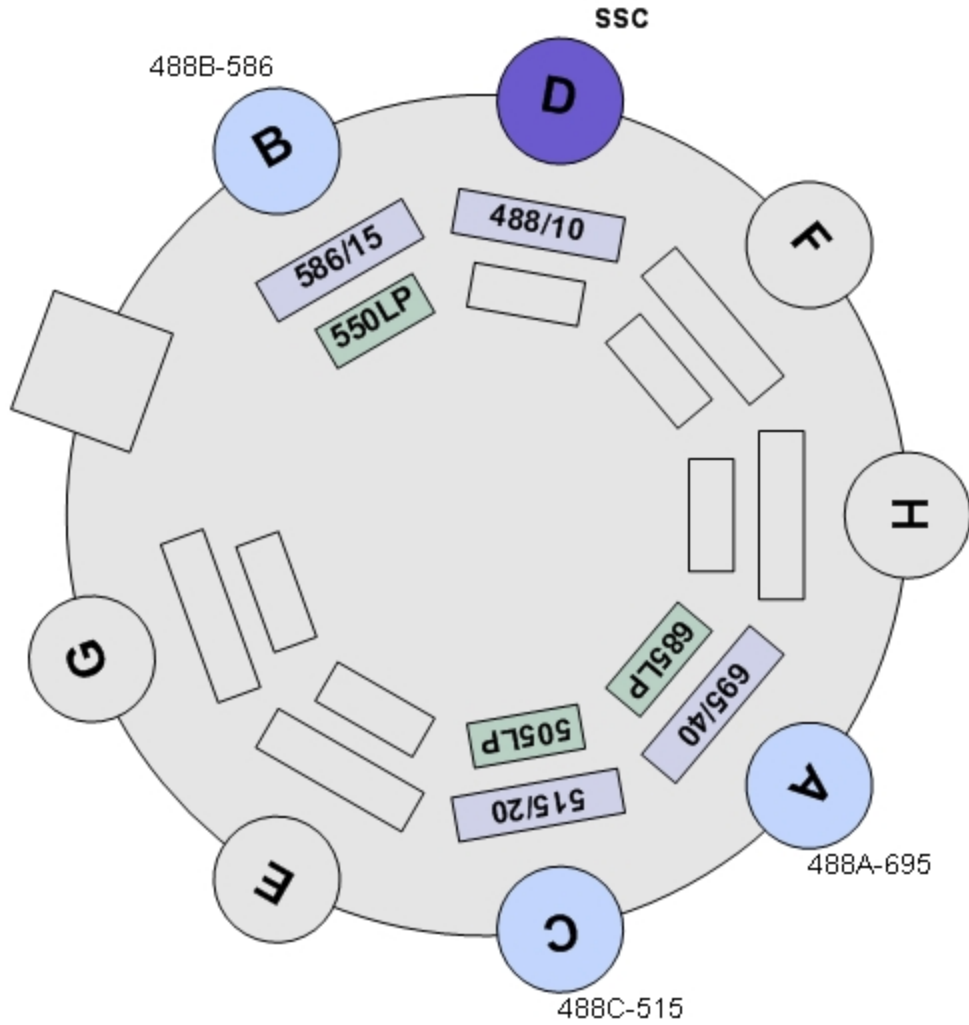


Violet Laser
(405nm)

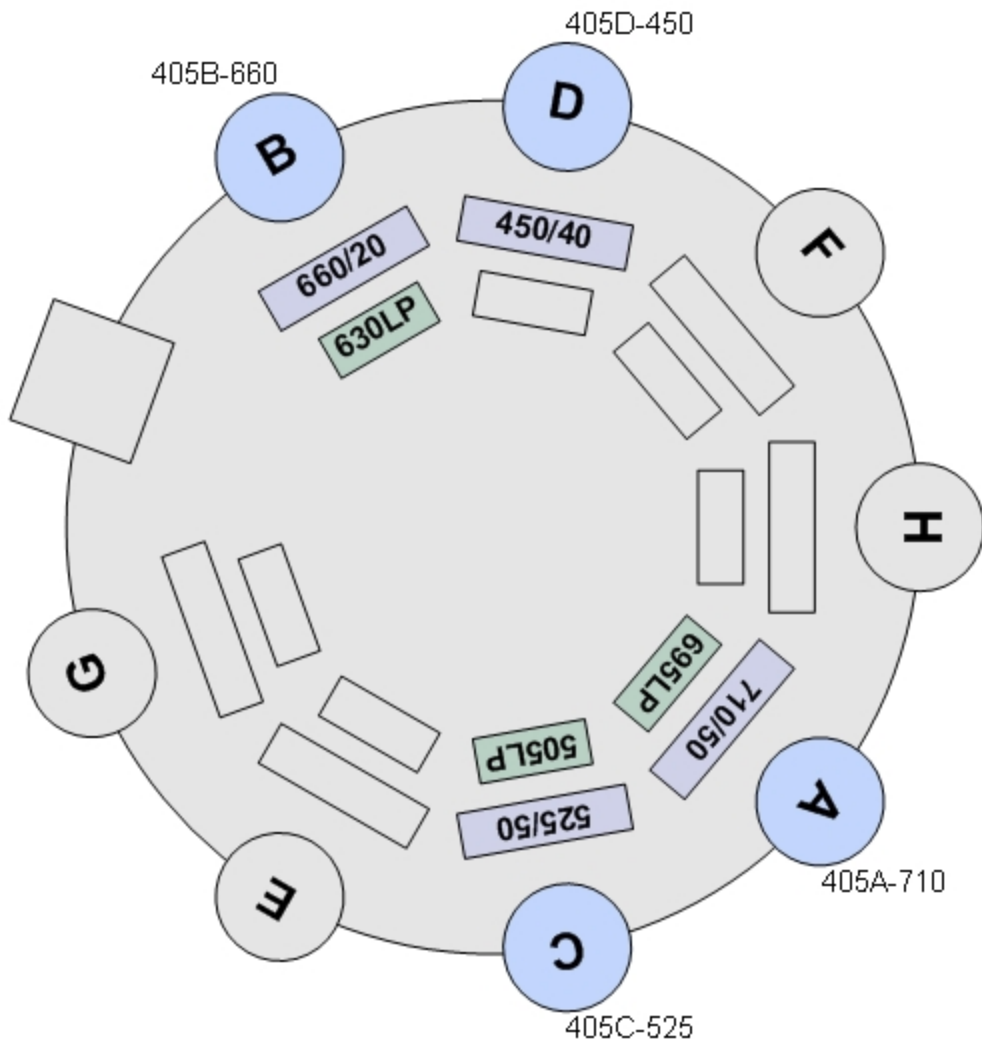


Red Laser
(633nm)

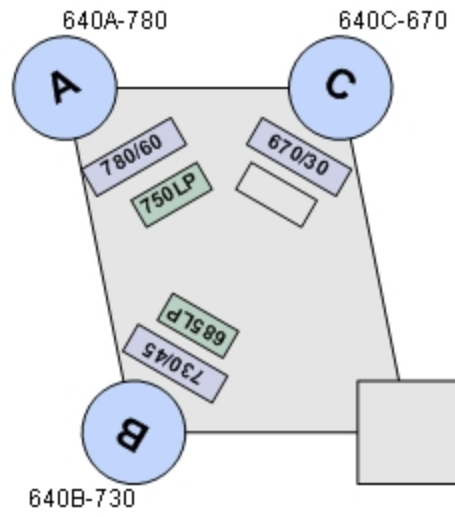

445 Blue-Violet Laser
(445nm)

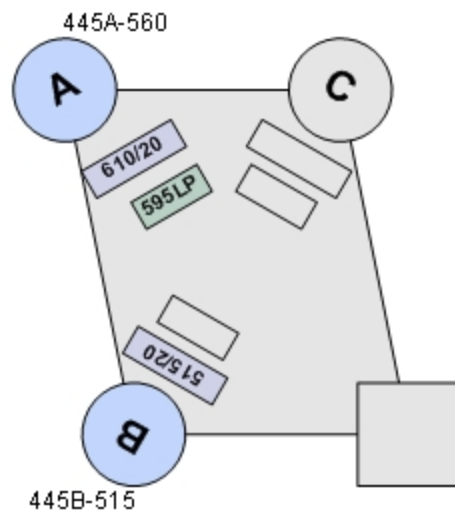

561 Yellow-Green Laser
(561nm)

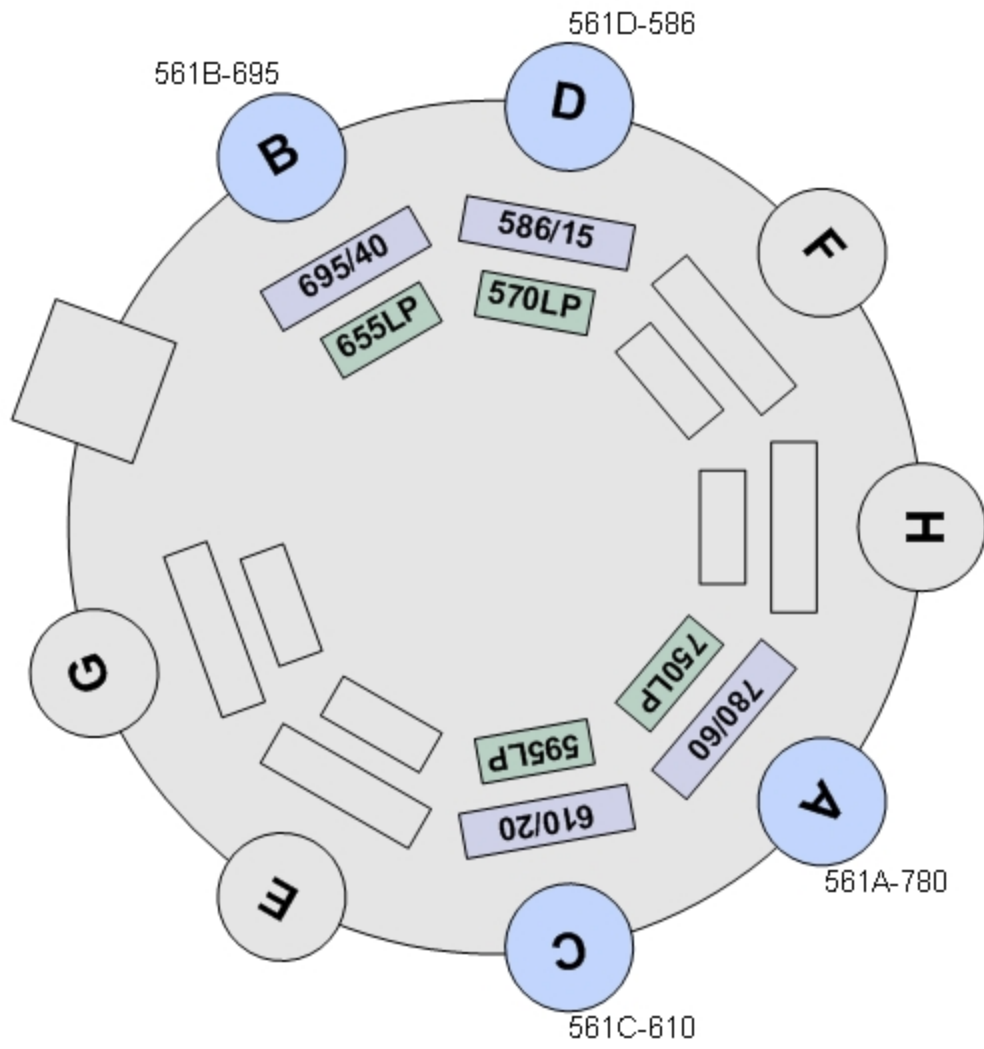

Comments: