


BD LSR II-1 DEFAULT 16 COLOR 2015_04_28


Cytometer: LSR II
Cytometer Name: LSR II
Serial Number: H48200001
Input Device: HTS
Window Extension: 10.00

User: Administrator
Institution: N/A
Software: BD FACSDiva 8.0.1
Date: 5/14/2015 11:04:41 AM


Blue Laser
(488nm)
FSC

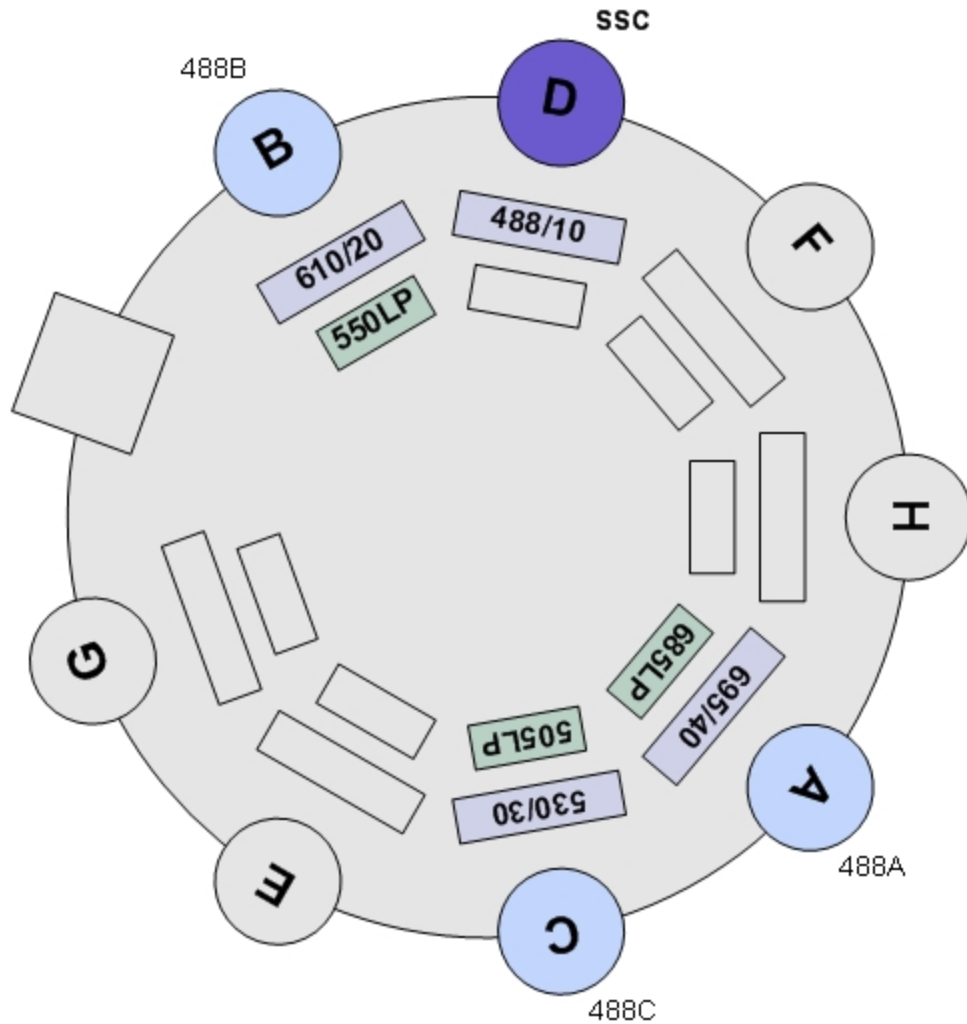


Violet Laser
(405nm)

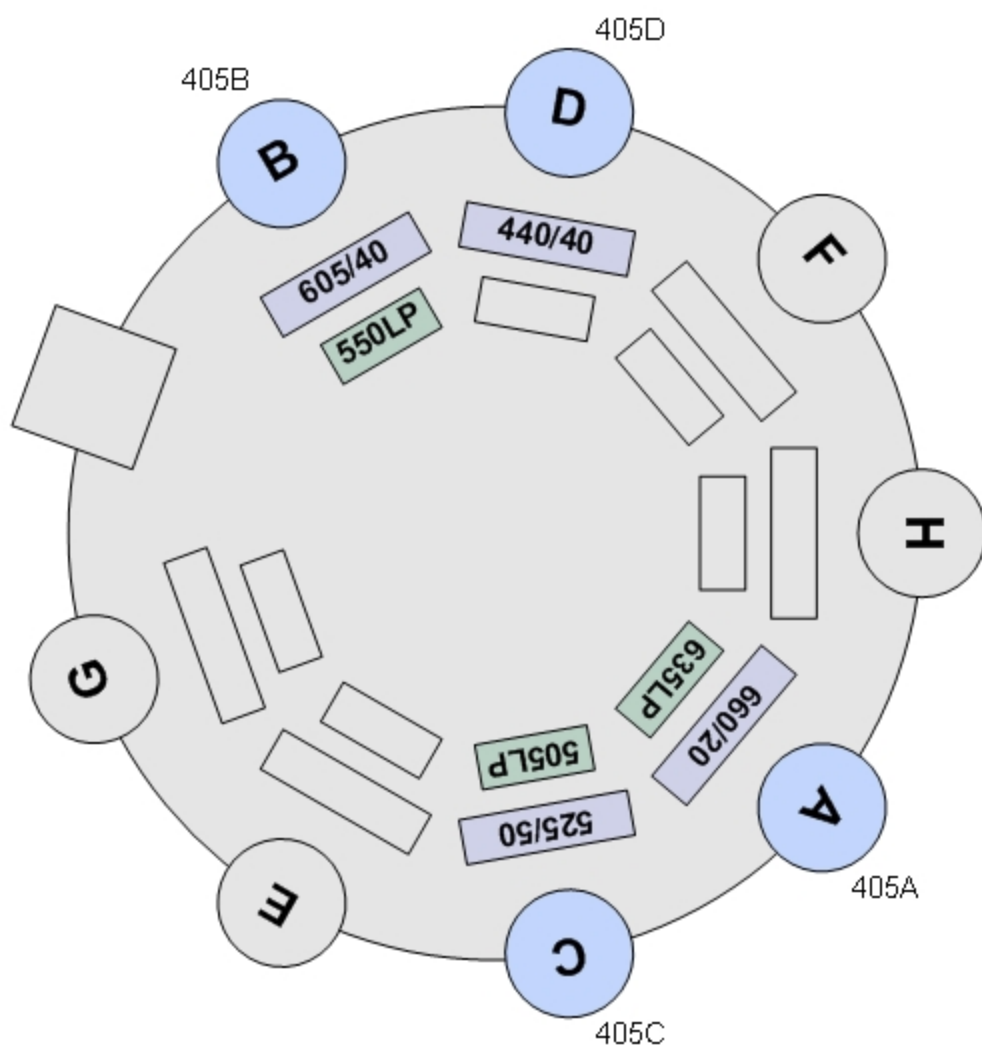


355 UV Laser
(355nm)

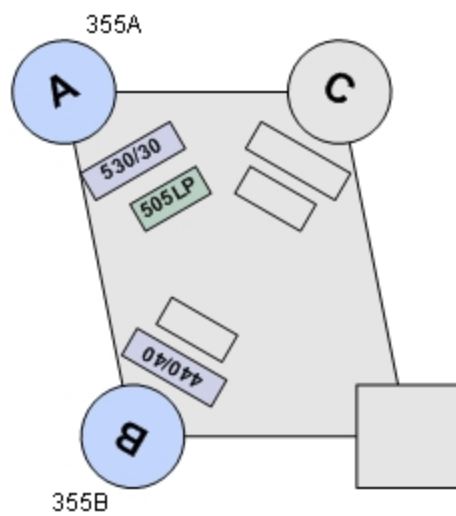

Red Laser
(633nm)

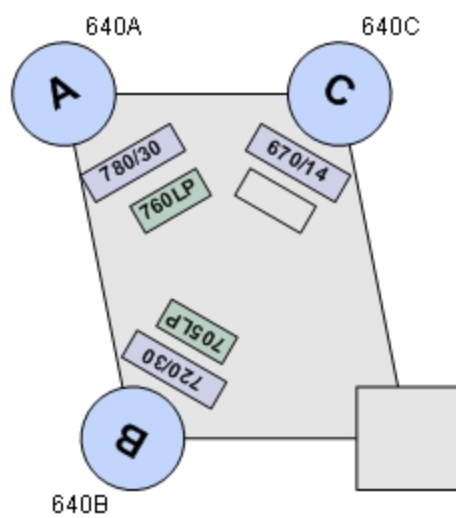

561 Yellow-Green Laser
(561nm)

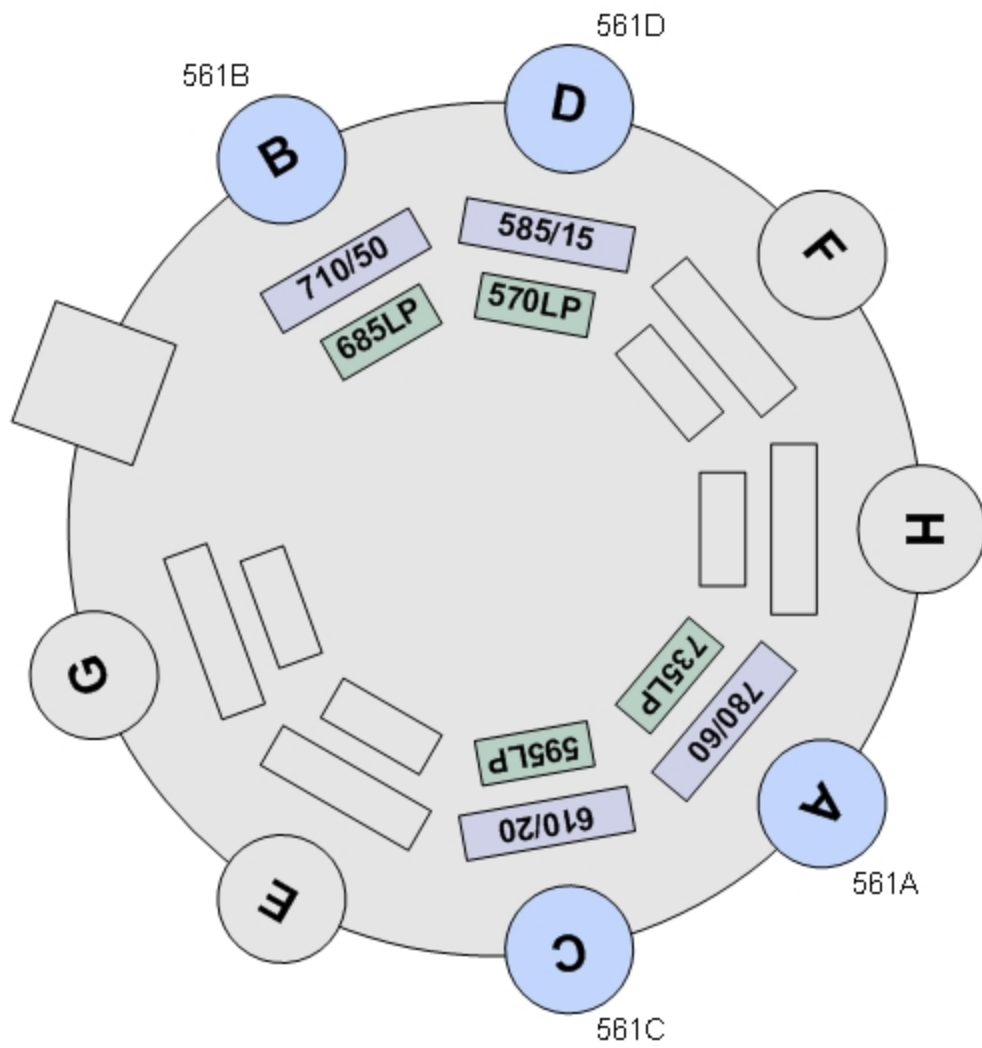

Comments: